


Update User's Guide for Measurement Data Handling (October 2025)

Sub-section On-Site Measurement Data

【Current version】

3. Only when explicitly instructed by the person in charge of the beamline, you may connect an internal storage device via SATA port to the PC or designated SATA port on the network drive installed at the beamline. Permissible internal storage devices must be brand-new and unopened until unsealed in the presence of the person in charge of the beamline. Any device that has been connected to another machine, even once, cannot be used with the beamline PC. Acceptable internal storage devices include hard disk drives (HDDs) and solid-state drives (SSDs).

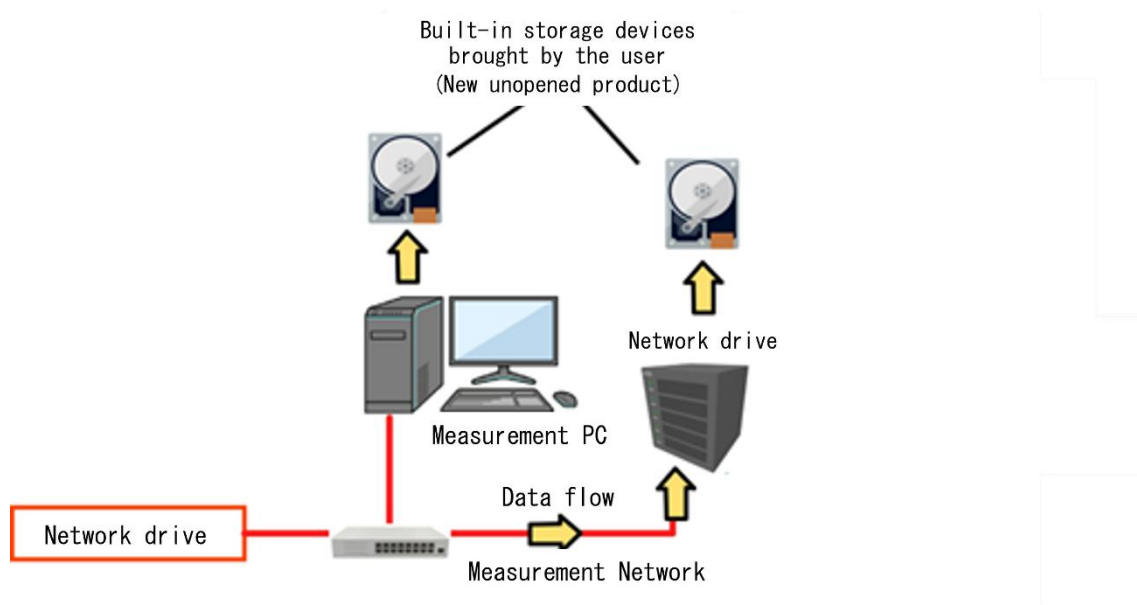


Prohibited Actions

Except for new, unopened storage devices verified by Beamline Staff, users must not use any storage device that has not undergone a security check for computer viruses.

【Update】

3. Only when explicitly instructed by the person in charge of the beamline, you may connect an internal storage device via SATA port to the PC or designated SATA port on the network drive installed at the beamline. Permissible internal storage devices must be pre-formatted. Acceptable internal storage devices include hard disk drives (HDDs) and solid-state drives (SSDs).

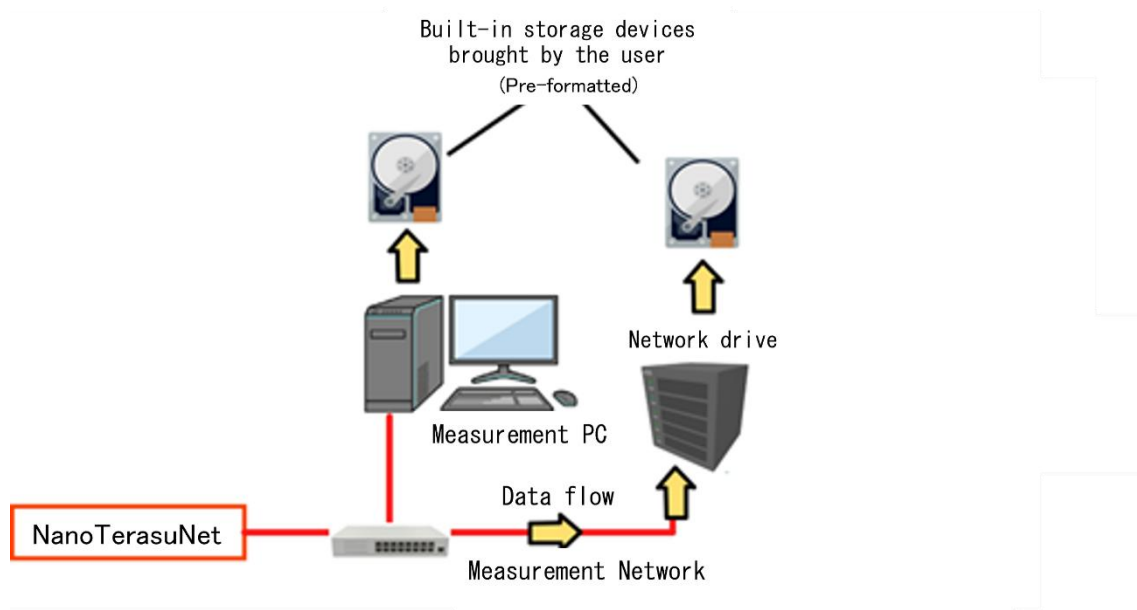

Prohibited Actions

Except for pre-formatted storage devices, users must not use any storage device that has not undergone a security check for computer viruses using the latest pattern files.